

FIG. 1

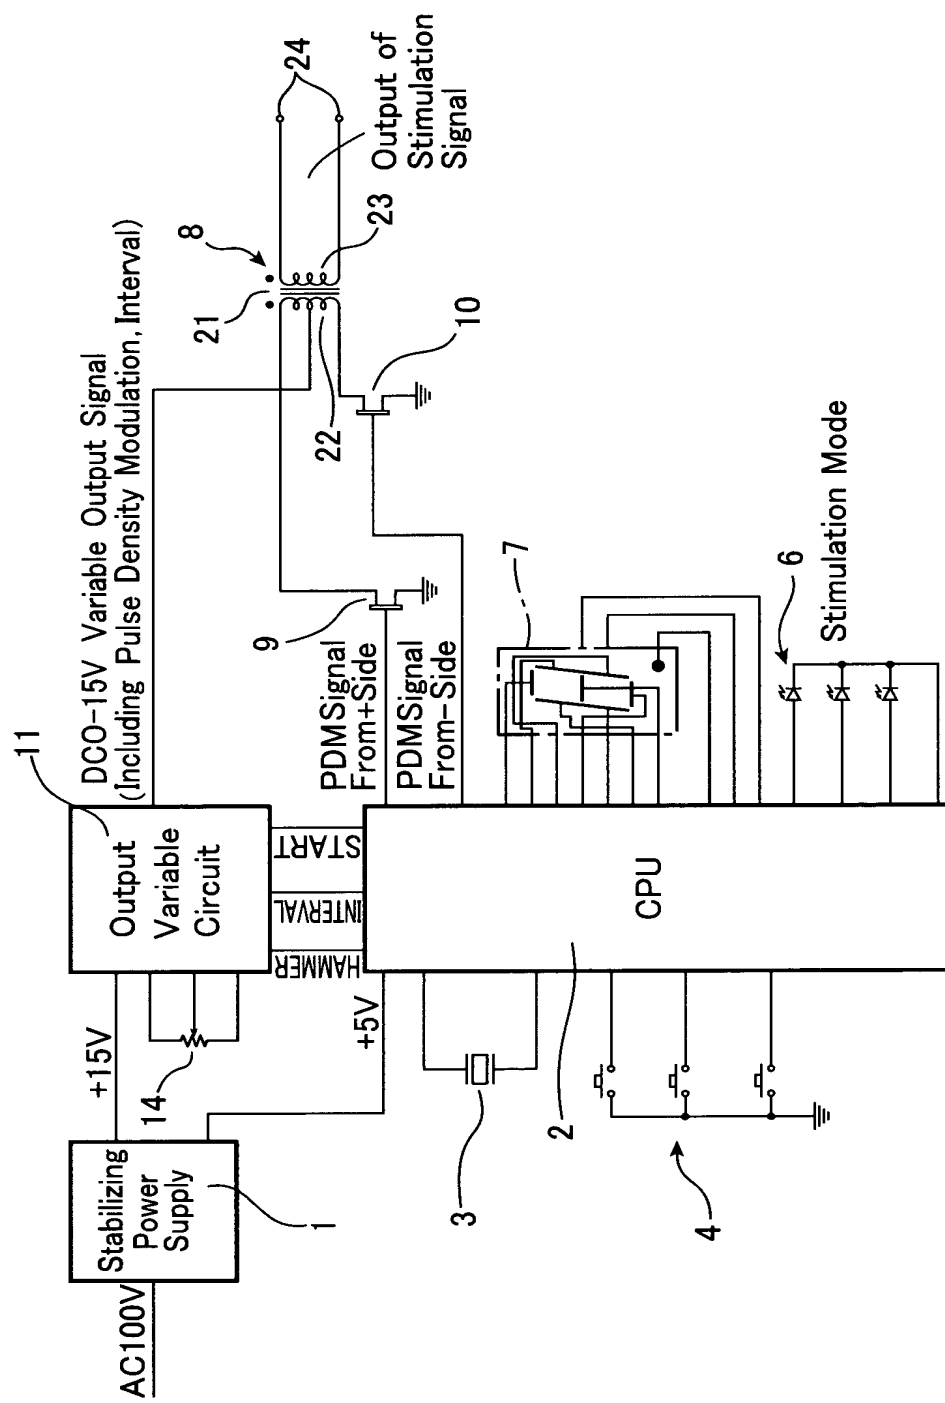


FIG. 2

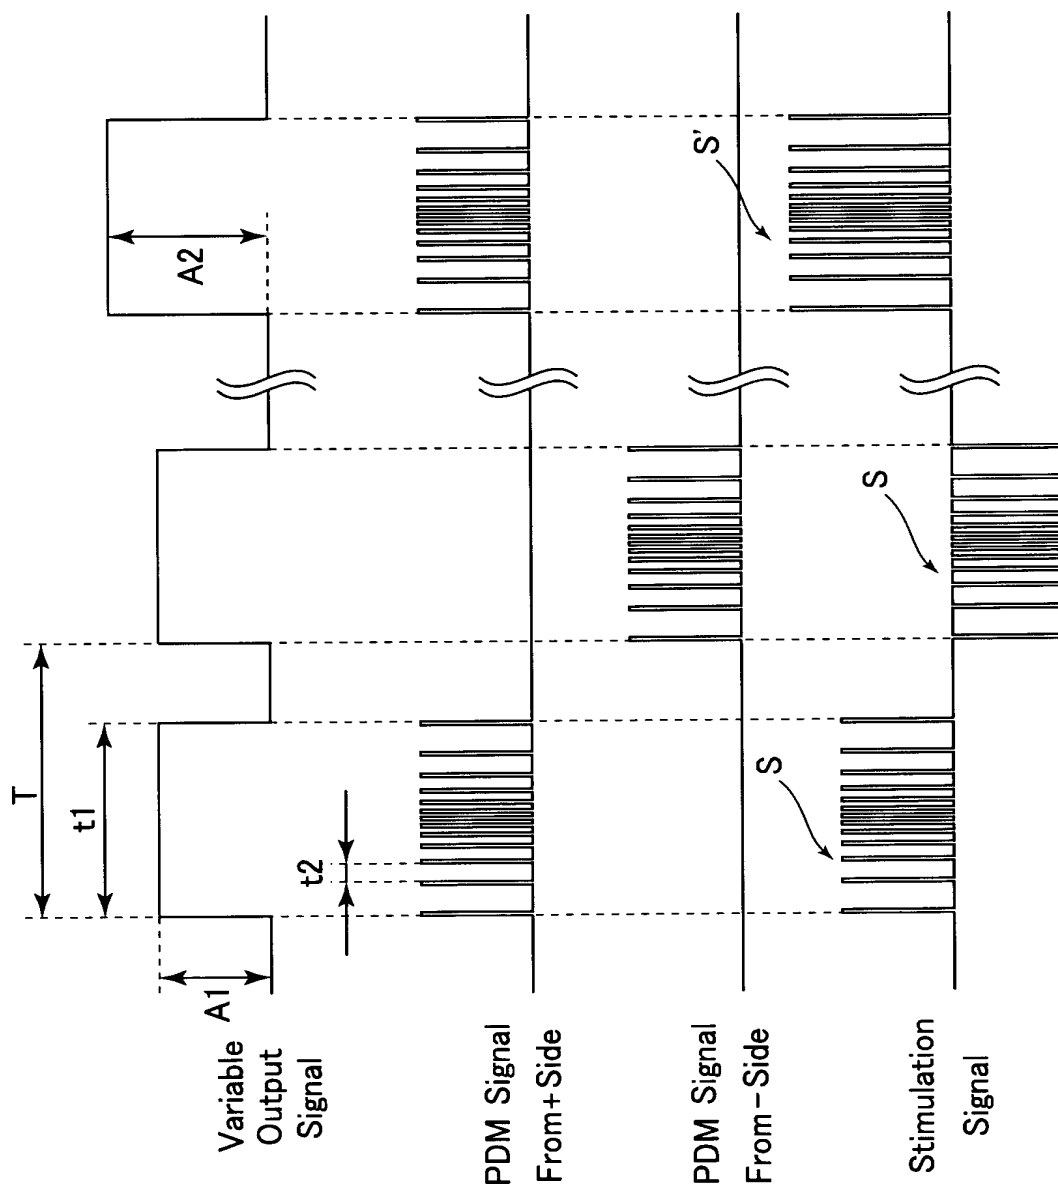


FIG. 3 Waveform in the case where the apparatus is connected to a 500 Ω resistor.

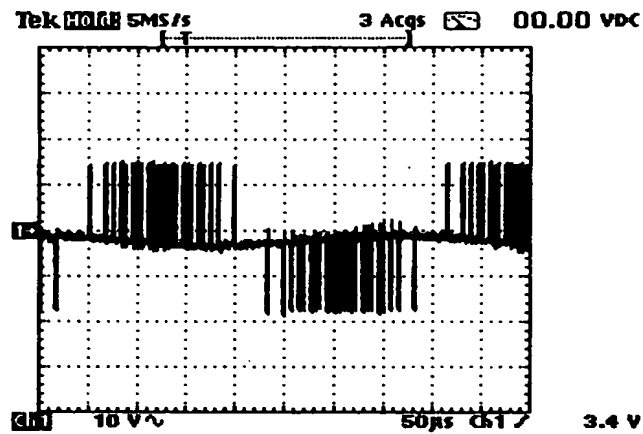


FIG. 4 Waveform showing enlarged half cycle waveforms in FIG.3.

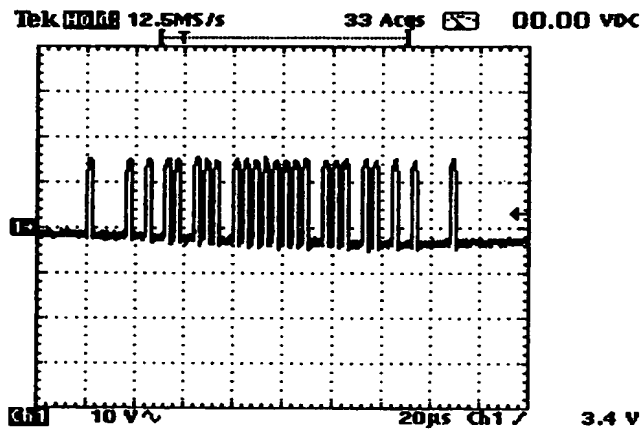


FIG. 5 Waveform in the case where the apparatus is attached to a human waist.

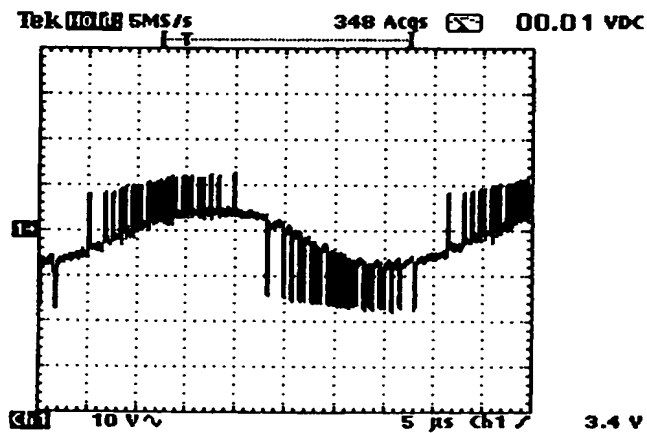


FIG. 6

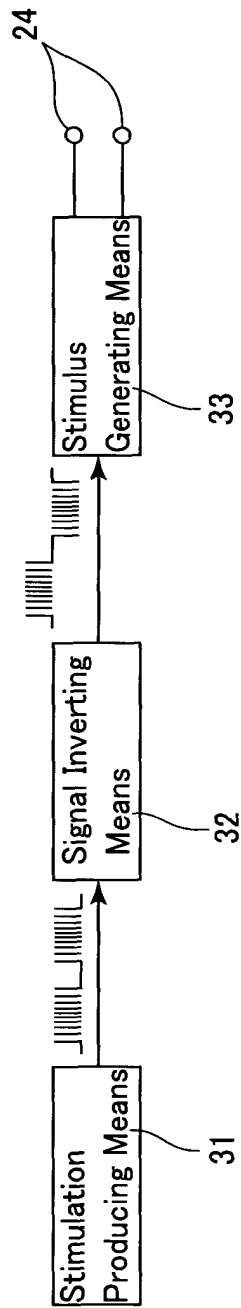


FIG. 7
(PRIOR ART)

